




JDENTAL CARE
just smile



MADE IN ITALY

Ø 2.75

Dental Implant
JD ICON[®] Ultra.S

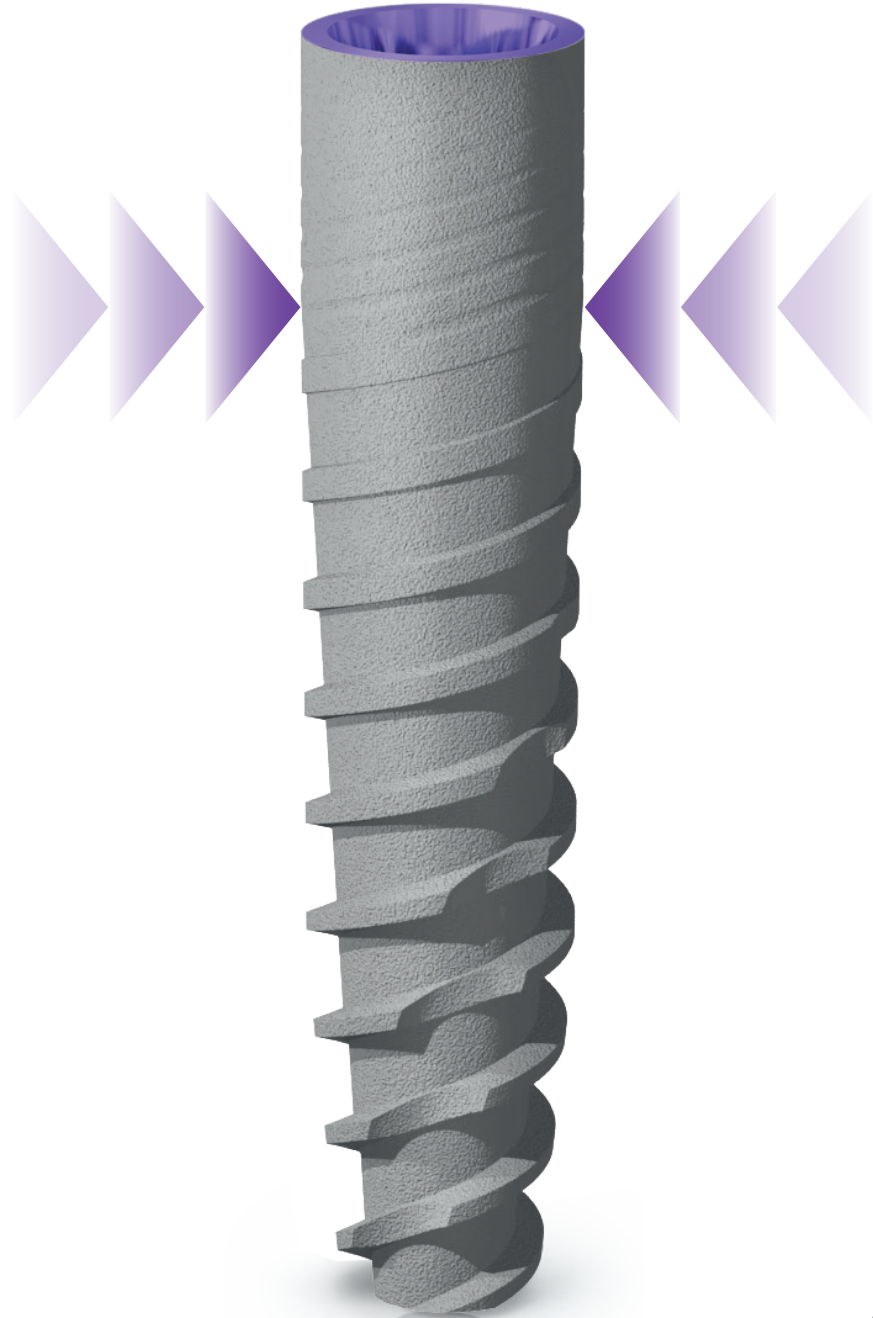


Smaller and Stronger.

JD ICON® ULTRA.S

SMALLER AND STRONGER

Ø 2.75

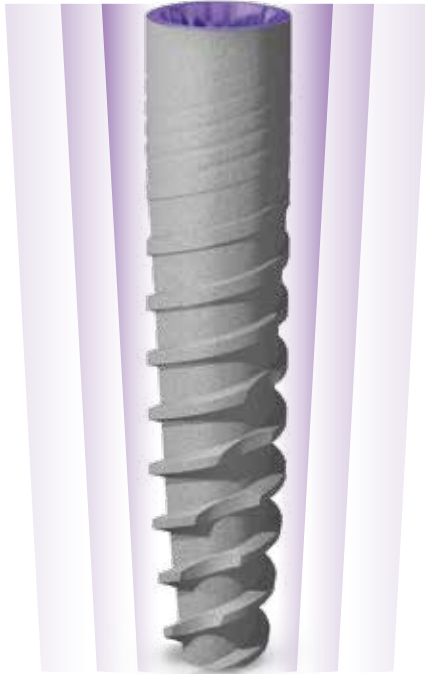

JDIcon Ultra S is a two-piece implant with 2.75mm diameter and internal conical connection.

It is the smallest implant with internal connection ever manufactured.

Despite its small diameter JDIcon Ultra.S provides a high implant strength due to its innovative fixture design and its tight conical connection.

The results of fatigue strength tests conducted on JDIcon Ultra S implant indicate that it is even stronger than implants with larger diameter. (see table below)


IMPLANT CONCEPT AND STRENGTH TESTS

JDIcon Ultra.S is ideal for areas with limited spaces, such as missing lateral incisors.

It is intended for use for single-tooth restoration and in implant fixed partial dentures (implant bridges) in incisors and canine areas.

In the premolar area, it is intended for use in implant fixed partial dentures (implant bridges) in patients with no parafunctional habits. In case of narrow ridge dimensions, a simplified surgical protocol in combination with the conservative dimensions of this dental implant facilitate the resolution of dental implant cases which would have otherwise required the use of bone augmentation and higher treatment costs.

MAXIMUM FATIGUE STRENGTH (N)

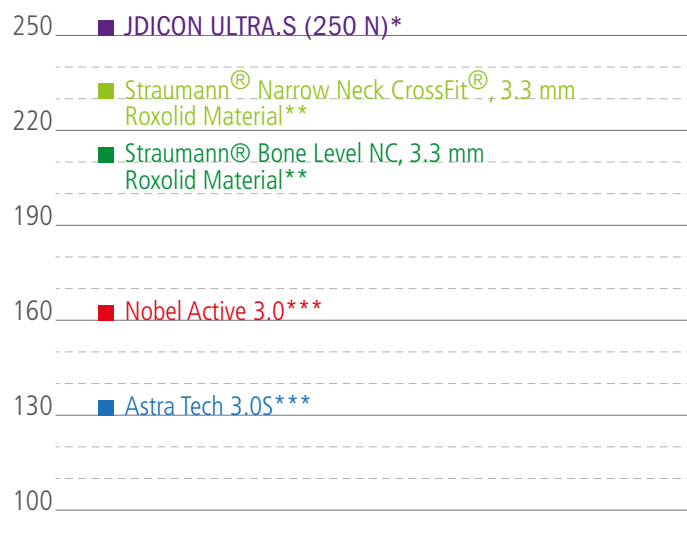

Fatigue strength is the maximum force an implant / abutment structure can survive for at least five million cycles. JDIcon Ultra.S has been tested according to ISO 14801 that is accepted by many regulatory agencies including FDA and Notified Bodies (CE).

*All tests on JDIcon Ultra S were conducted by Politecnico di Milano University.

** Values declared by Straumann

*** Values declared by Nobel Biocare



POLITECNICO DI MILANO

JD ICON®ULTRA.S

IMPLANT MEASURES AND LENGTHS

The JDICON®ULTRA.S dental implant is available in the lengths shown in this chart:

IMPLANT DIAMETER	TIP DIAMETER	ABUTMENT INTERFACE	PLATFORM DIAMETER	LENGTH
∅ 2,75	∅ 2,0	∅ 2,3	∅ 2,75	8 10 11,5 13 15



Note: All dimensions are expressed in millimeters.

DRILLING SEQUENCE

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability of the implant.

IMPLANT DIAMETER	SOFT BONE TYPE IV	MEDIUM BONE TYPE II-III	DENSE BONE TYPE I
∅ 2,75	1,5	2,0	2,0
	2,0	2,4	2,4 2,8*


* Until the first laser mark

Note: All dimensions are expressed in millimeters.

Important:

JDIcon Ultra S Implant is designed to withstand a maximum insertion torque of 60 Ncm.

The JDIcon Ultra S prosthetic screw is developed for a maximum insertion torque of 20 Ncm.

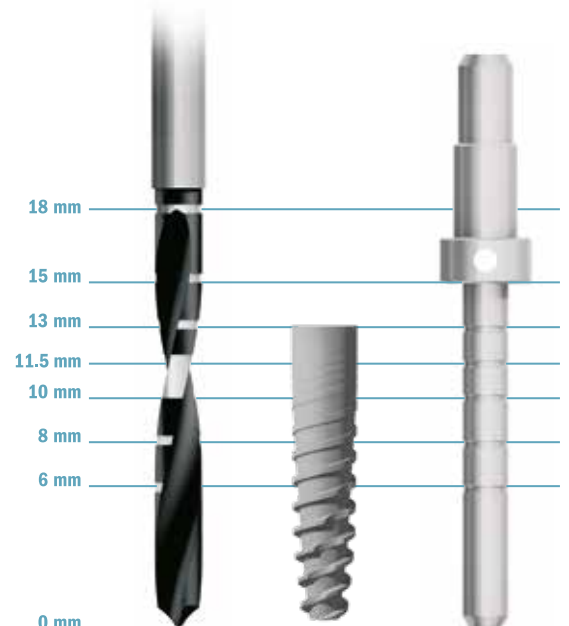

JD ICON® ULTRA.S

PRODUCT CATALOGUE

Implants

Ø 2,75

IC27080

IC27100

IC27115

IC27130

IC27150

JDIcon® Ultra.S Ø 2.75 L 8

JDIcon® Ultra.S Ø 2.75 L 10

JDIcon® Ultra.S Ø 2.75 L 11.5

JDIcon® Ultra.S Ø 2.75 L 13

JDIcon® Ultra.S Ø 2.75 L 15



Cover Screw

ISCS

Cover screw JDIcon® Ultra.S



Healing Abutment

ISHA323

ISHA325

ISHA327

Healing Abutment Ø 3.2 H 3.0 JDIcon® Ultra.S

Healing Abutment Ø 3.2 H 5.0 JDIcon® Ultra.S

Healing Abutment Ø 3.2 H 7.0 JDIcon® Ultra.S



ISHA403

ISHA405

ISHA407

Healing Abutment Ø 4.0 H 3.0 JDIcon® Ultra.S

Healing Abutment Ø 4.0 H 5.0 JDIcon® Ultra.S

Healing Abutment Ø 4.0 H 7.0 JDIcon® Ultra.S



Impression Copings

OPEN TRAY

ISICOT32C

ISICOT40C

Impression coping open tray Ø 3.2 JDIcon® Ultra.S

Impression coping open tray Ø 4.0 JDIcon® Ultra.S



CLOSED TRAY

ISICCT32C

ISICCT40C

Impression coping closed tray Ø 3.2 JDIcon® Ultra.S

Impression coping closed tray Ø 4.0 JDIcon® Ultra.S

Prosthetic Screw

ISS

ISSA

Abutment screw JDIcon® Ultra.S

Abutment screw angulated JDIcon® Ultra.S

Torque recommended 20 Ncm



Temporary Abutment

ISTAEC

Temporary abutment engaging JDIcon® Ultra.S



GP Abutment

ISGP32C

ISGP40C

GP abutment Ø 3.2 JDIcon® Ultra.S

GP abutment Ø 4.0 JDIcon® Ultra.S

Torque recommended 20 Ncm




Wax up Abutment:

ISWAEC

Wax up abutment engaging JDIcon® Ultra.S

Torque recommended 20 Ncm




Straight Abutment:

ISSA4020C
ISSA4040C

Straight abutment Ø 4.0 H 2.0 JDIcon® Ultra.S
Straight abutment Ø 4.0 H 4.0 JDIcon® Ultra.S

Torque recommended 20 Ncm



Angulated Abutment:

IS15GPA40C

Angulated abutment 15° Ø 4.0 JDIcon® Ultra.S

Torque recommended 20 Ncm



TiBase, JDScanBody and Implant Replica CAD CAM:

ISSBCEC

JDScanBody for JDIcon® Ultra.S

ISTIBC

TiBase engaging JDIcon® Ultra.S

EVSCBOW

ScanBody for TiBase

ISANC

Implant Replica CAD CAM for JDIcon® Ultra.S

ISPMNC

JD Pre-milled blanks and abutment screw JDIcon® Ultra.S



Torque recommended 20 Ncm

Ball Abutment:

ISBA15
ISBA30
ISBA50

Ball abutment H 1.5 JDIcon® Ultra.S
Ball abutment H 3.0 JDIcon® Ultra.S
Ball abutment H 5.0 JDIcon® Ultra.S

Torque recommended 20 Ncm



Note: All the prosthetic components on ball abutments are the same as JDEvolution® implant line.

Implant Replica:

ISAN

Implant replica JDIcon® Ultra.S



Implant and Prosthetic Drivers:

ISID

Implant Driver JDIcon® Ultra.S

ISIDL

Implant Driver Long JDIcon® Ultra.S

EVSDPF15

Screwdriver hex 1.20 for torque wrench L15

EVSDPF20

Screwdriver hex 1.20 for torque wrench L20

EVSDPF25

Screwdriver hex 1.20 for torque wrench L25

EVSDPF35

Screwdriver hex 1.20 for torque wrench L35

EVSDCAF

Screwdriver torque wrench Conical Abutment

EVSDP20

Screwdriver hex 1.20 machine prosthetic L20

EVSDP25

Screwdriver hex 1.20 machine prosthetic L25

EVSDP30

Screwdriver hex 1.20 machine prosthetic L30

EVSDCA

Screwdriver machine Conical Abutment

EVSDPF25A

Screwdriver screw angulated for torque wrench L25

EVSDPF30A

Screwdriver screw angulated for torque wrench L30





JDENTALCARE

www.jdentalcare.com